

PRIOR ART

Fig. 1

FIG. 2

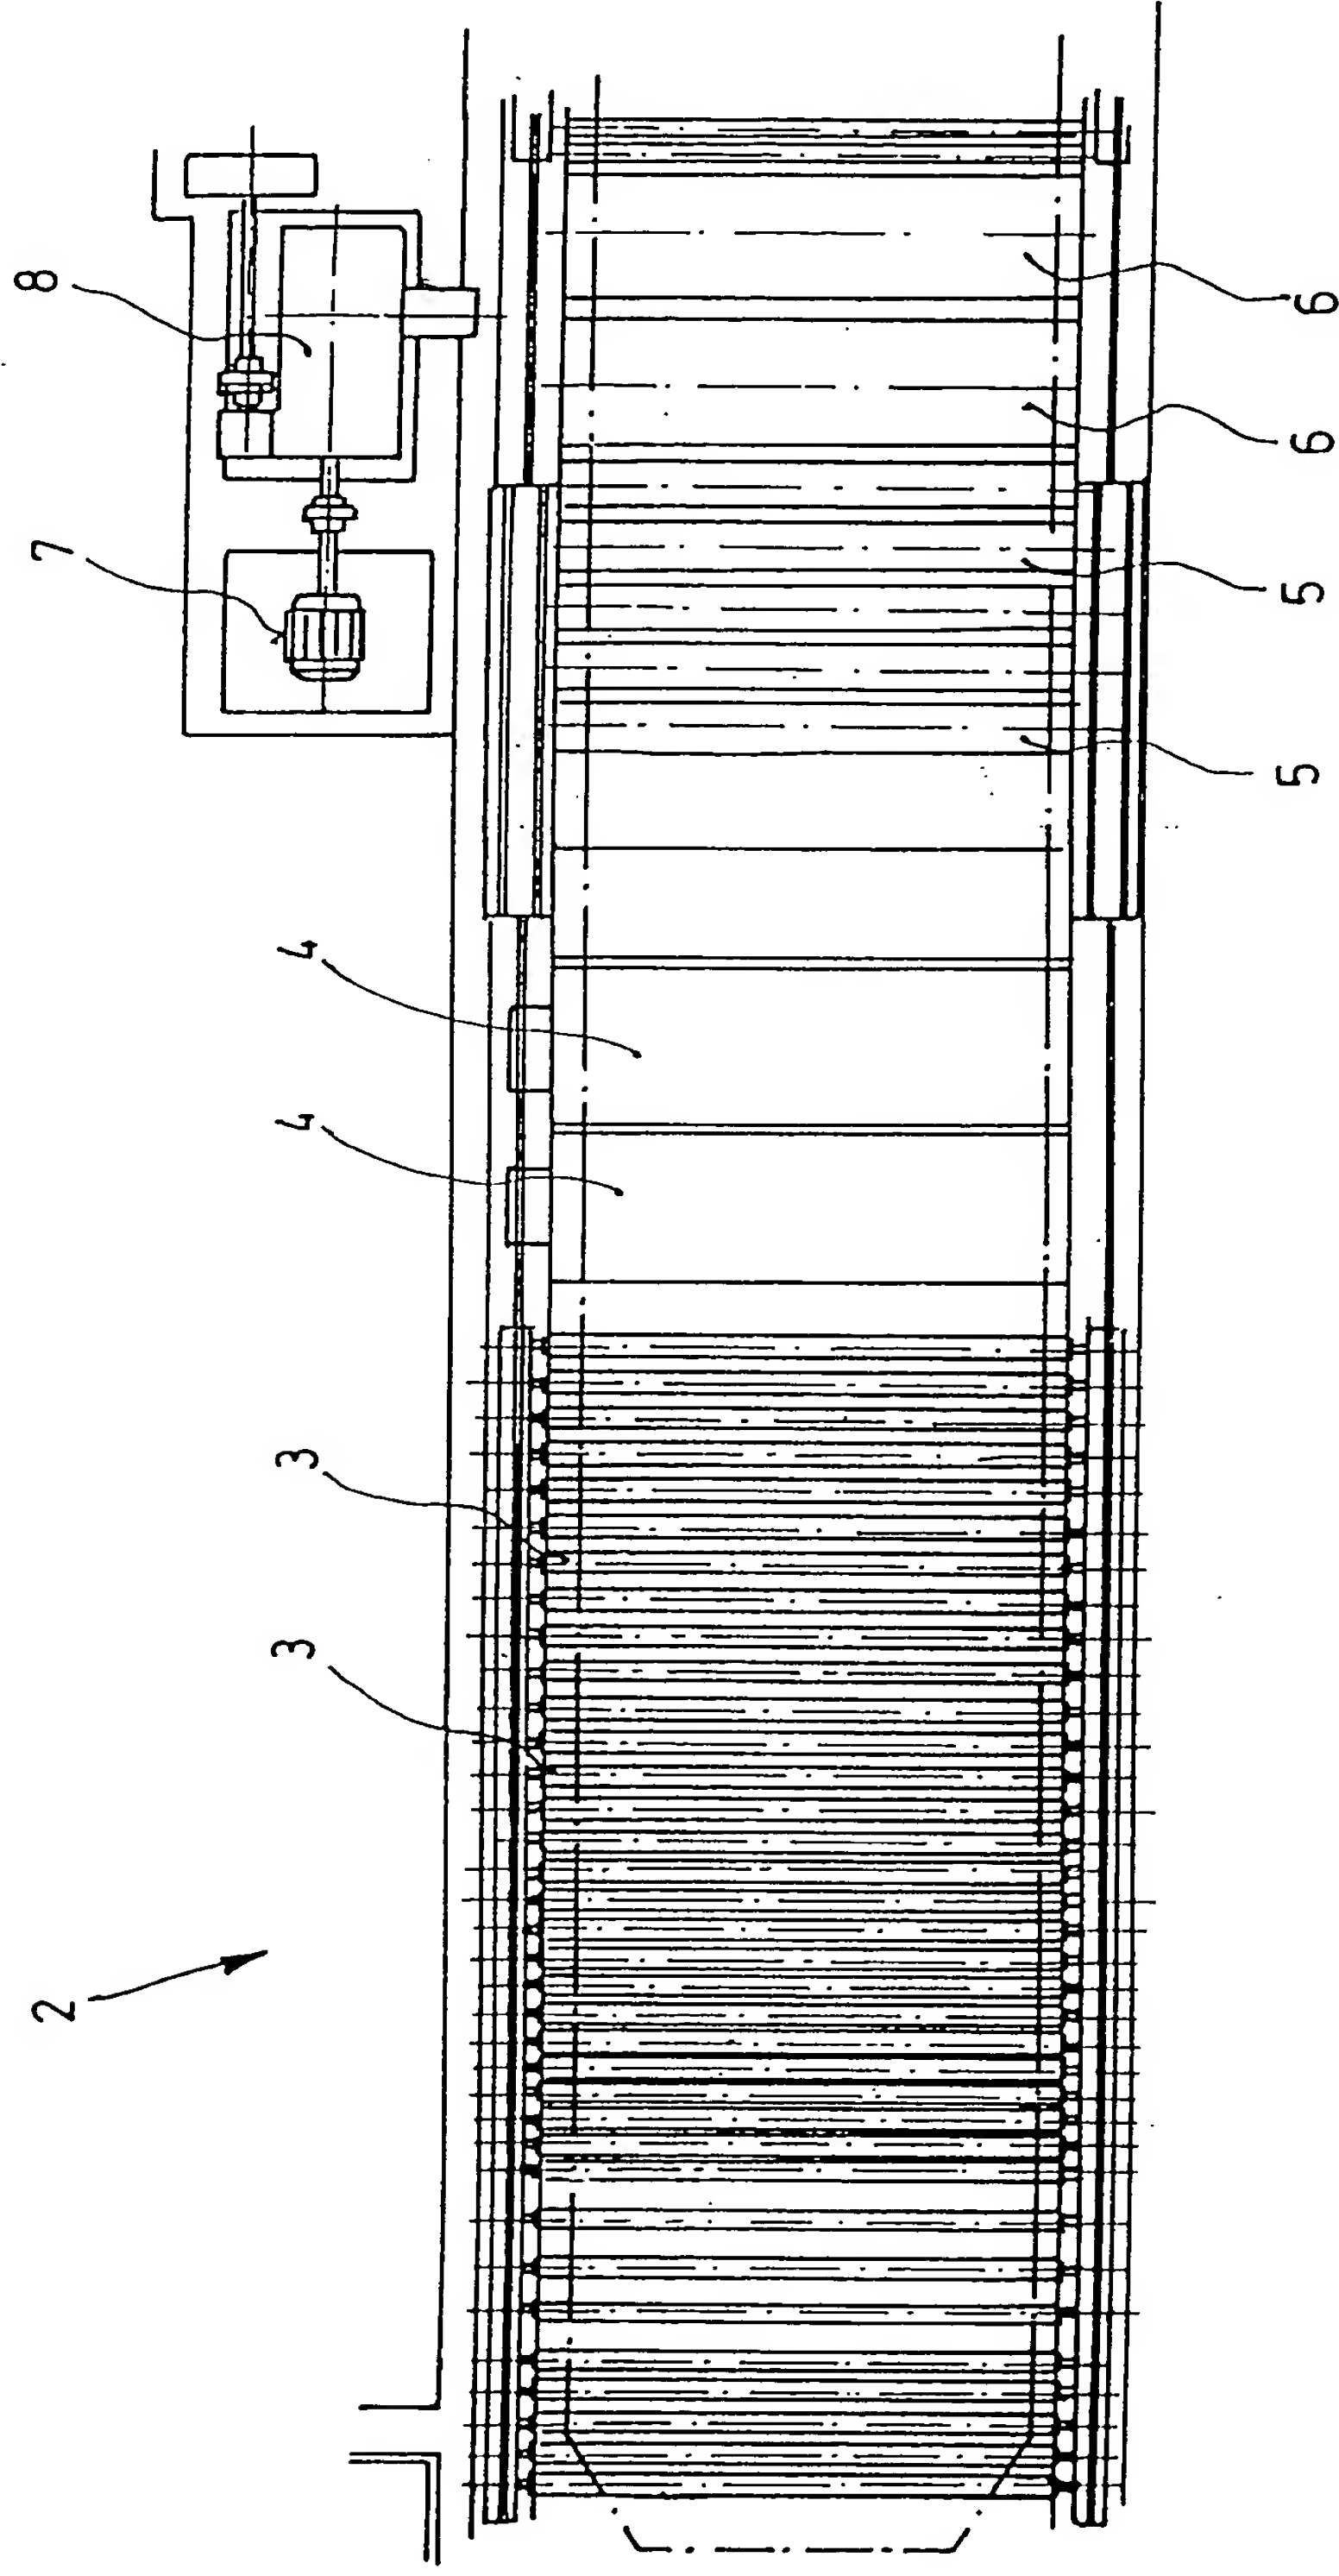


Fig. 2

PRIOR ART

Fig. 3

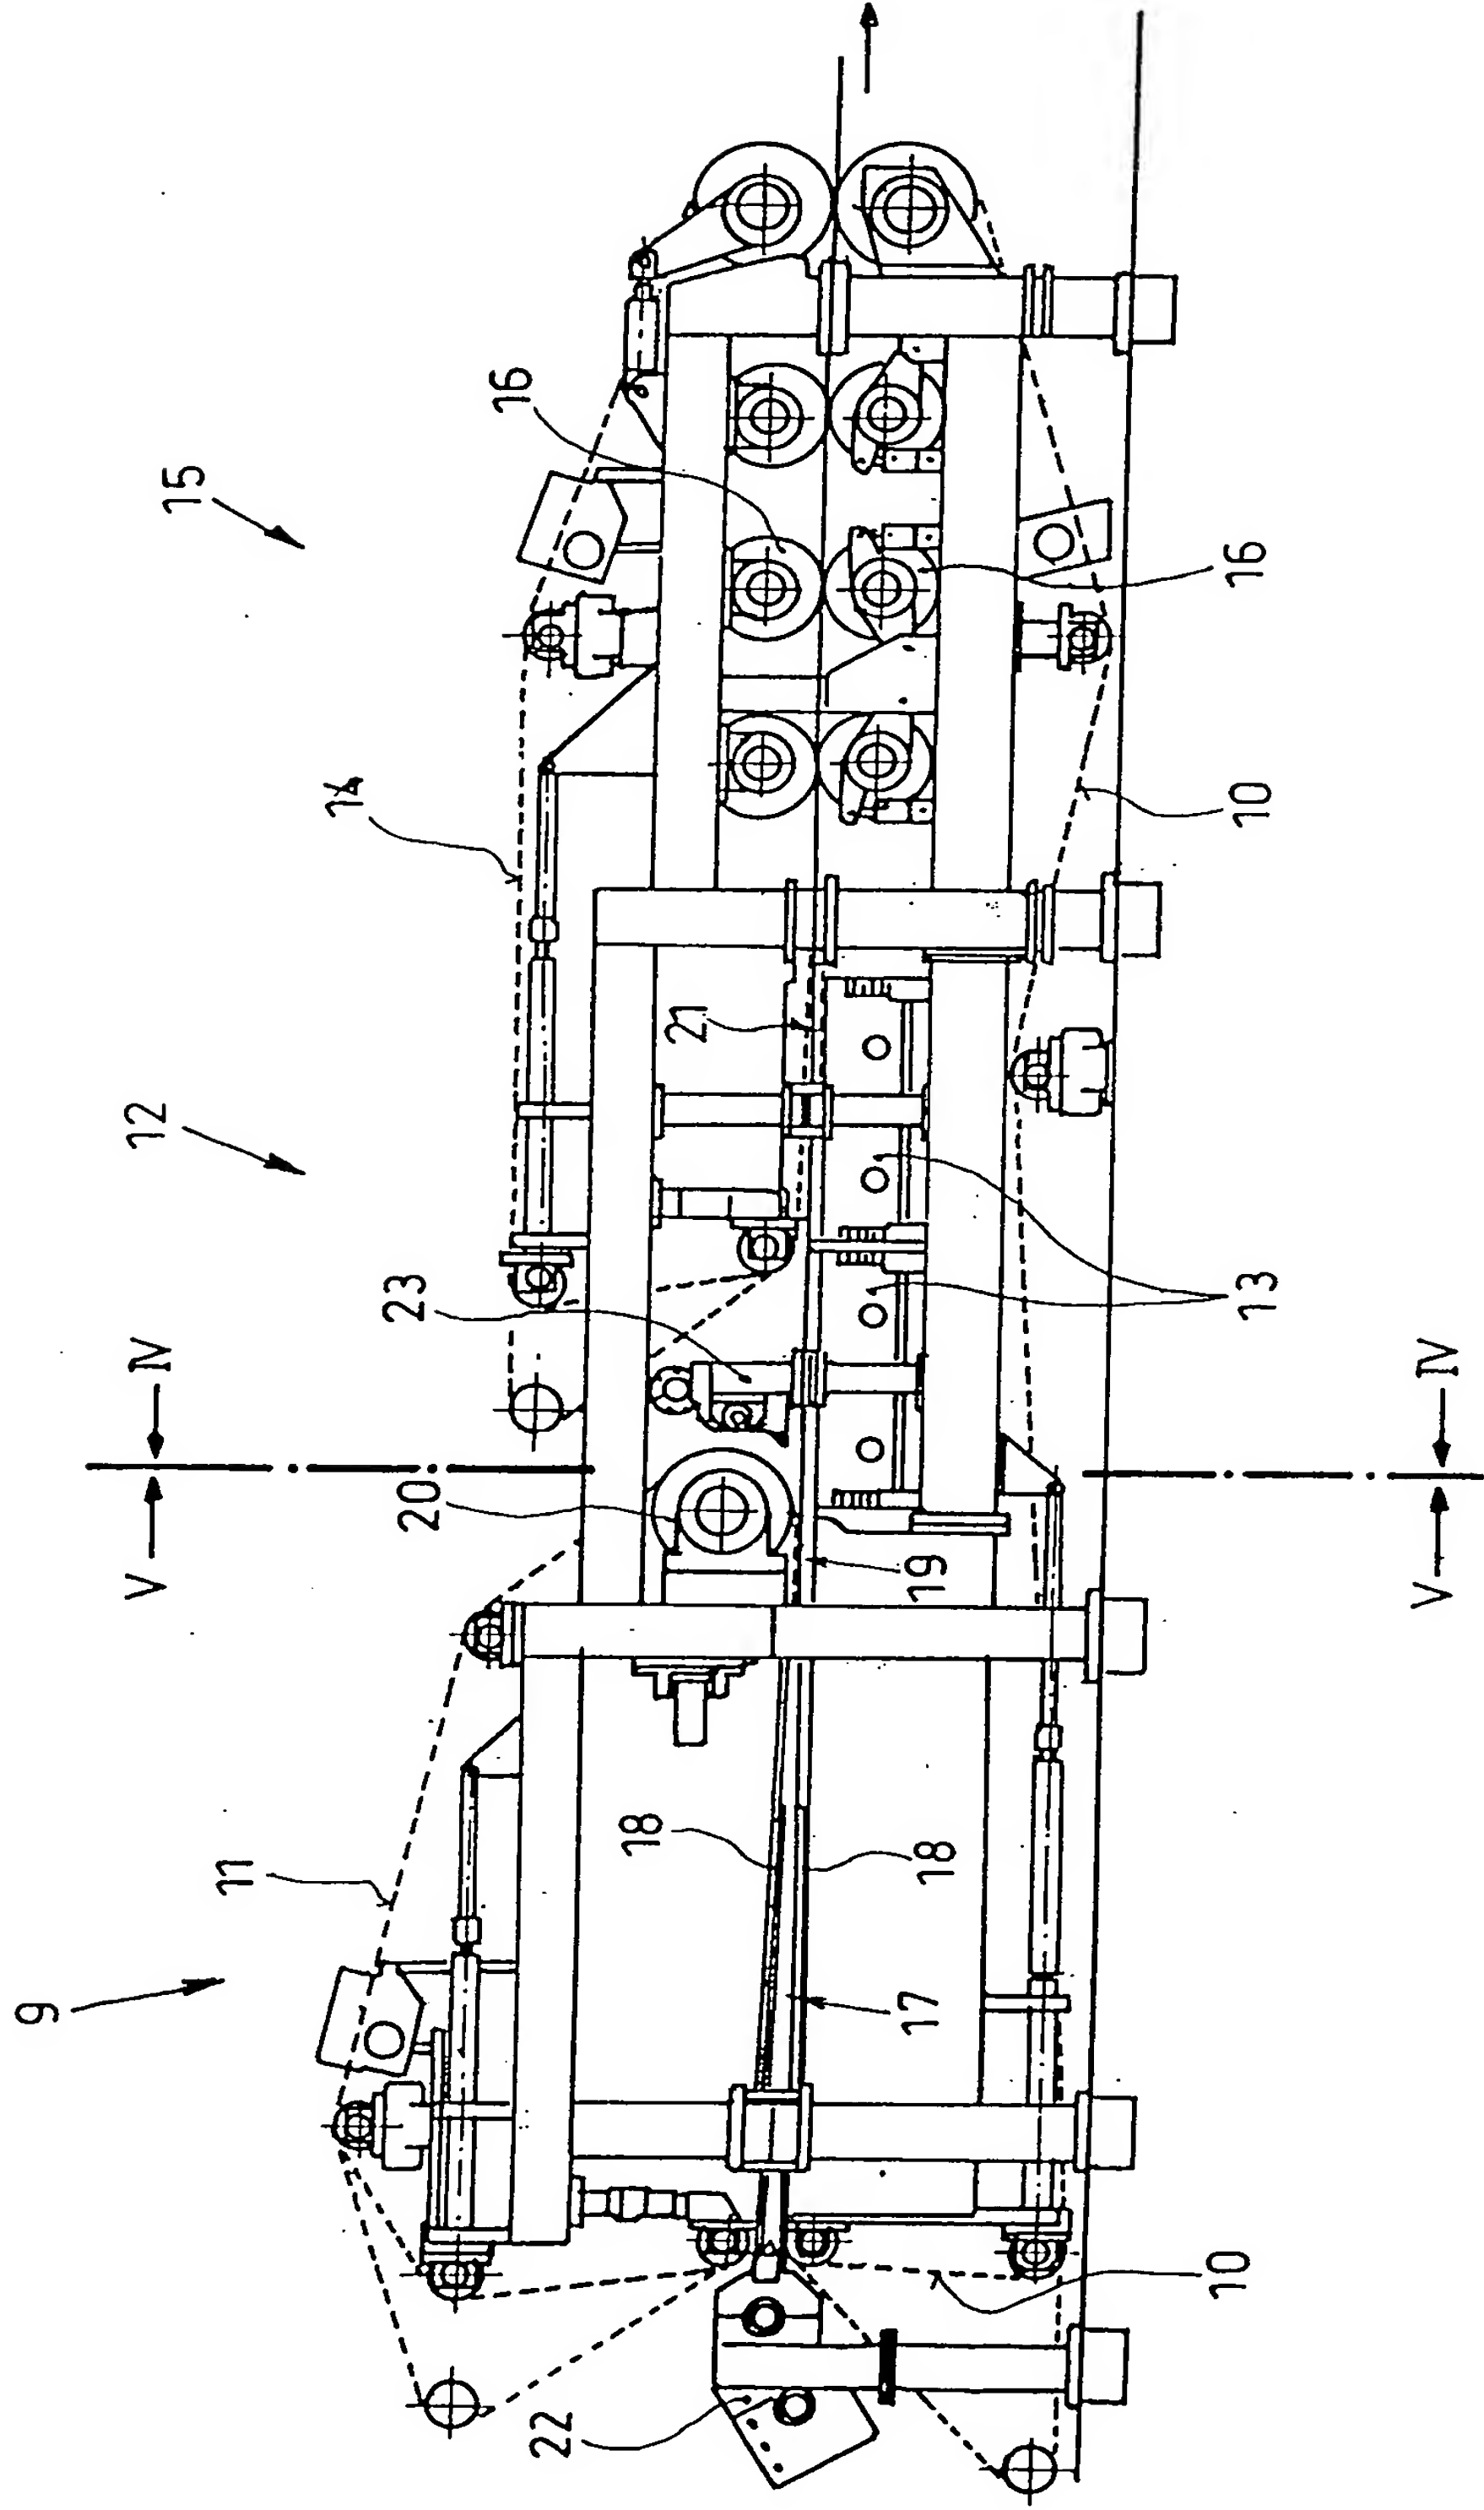


Fig. 3

Fig. 4 is a cross-sectional view of the device taken along line A-A of Fig. 1.

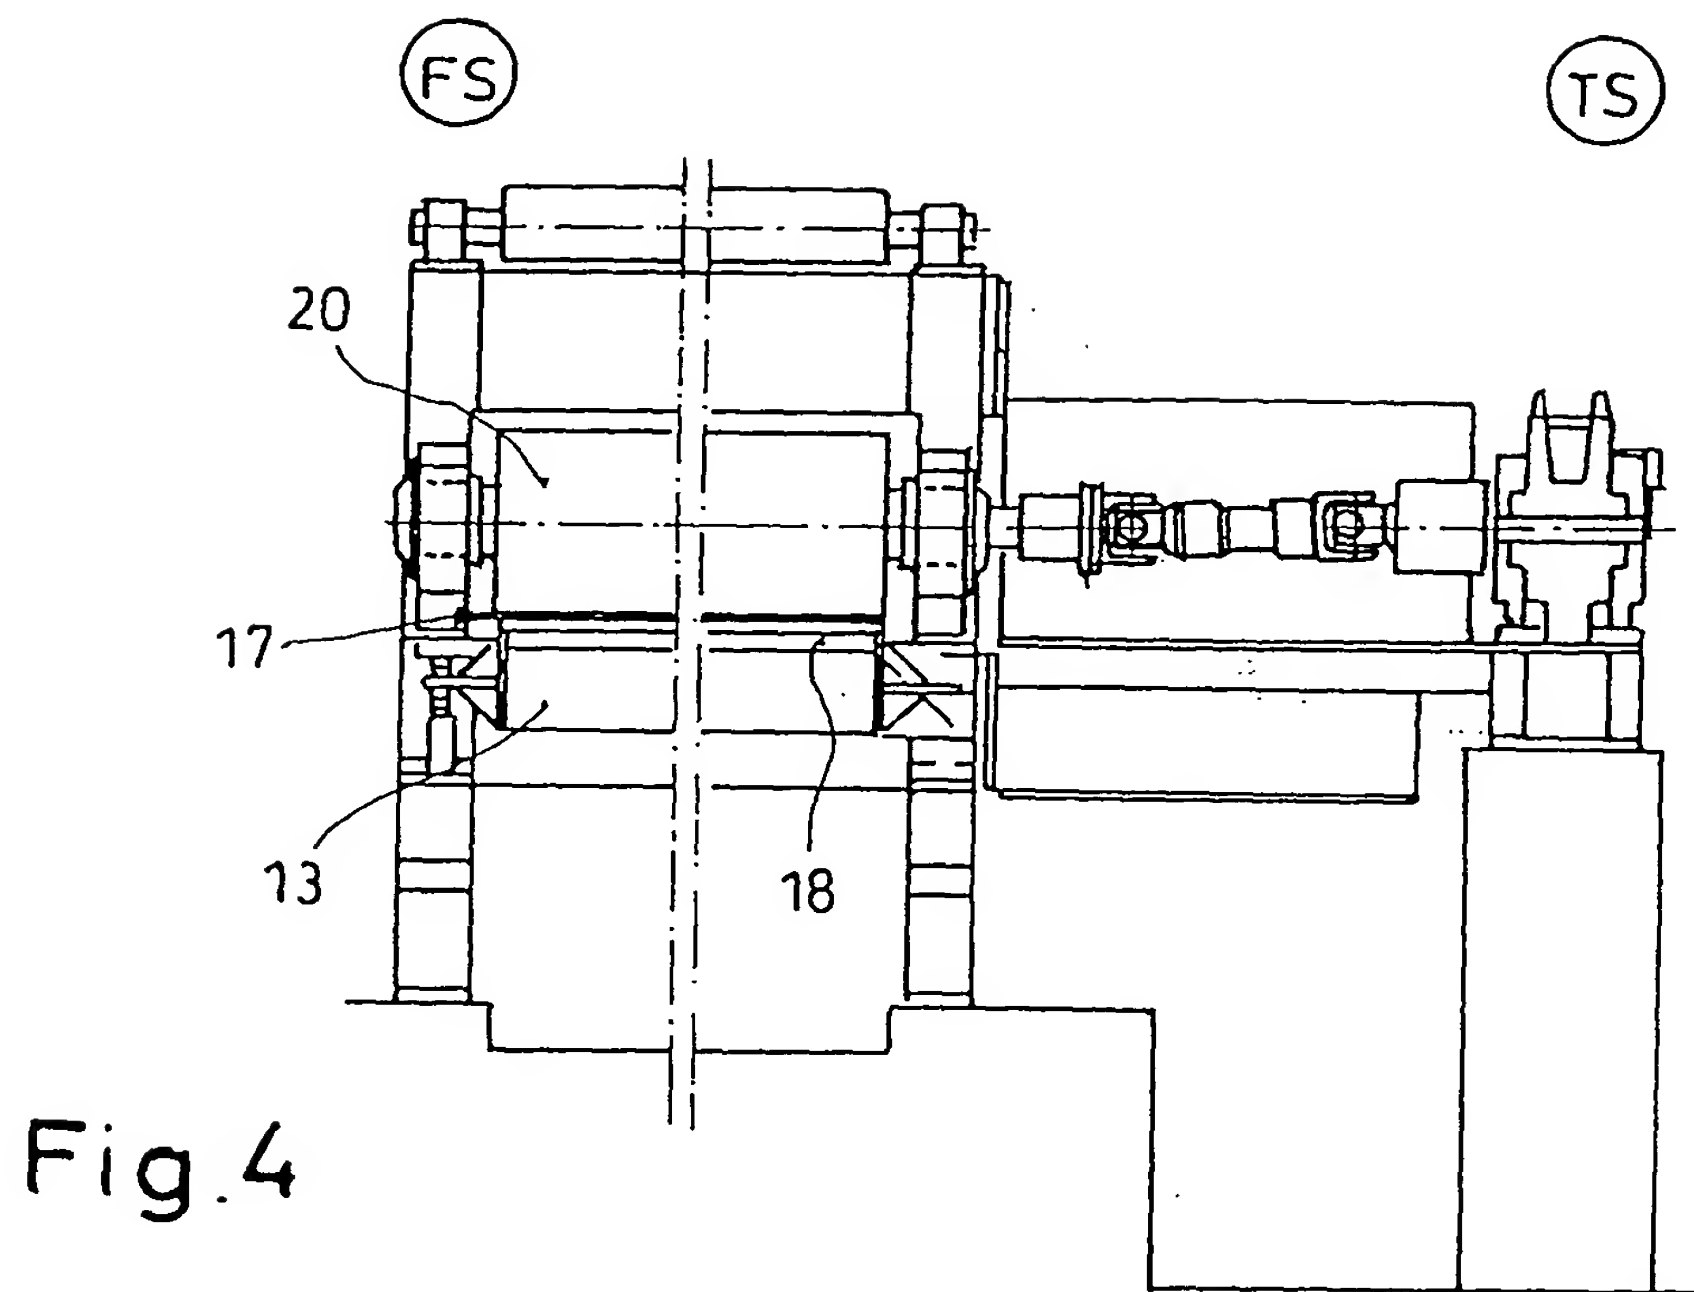


Fig. 4

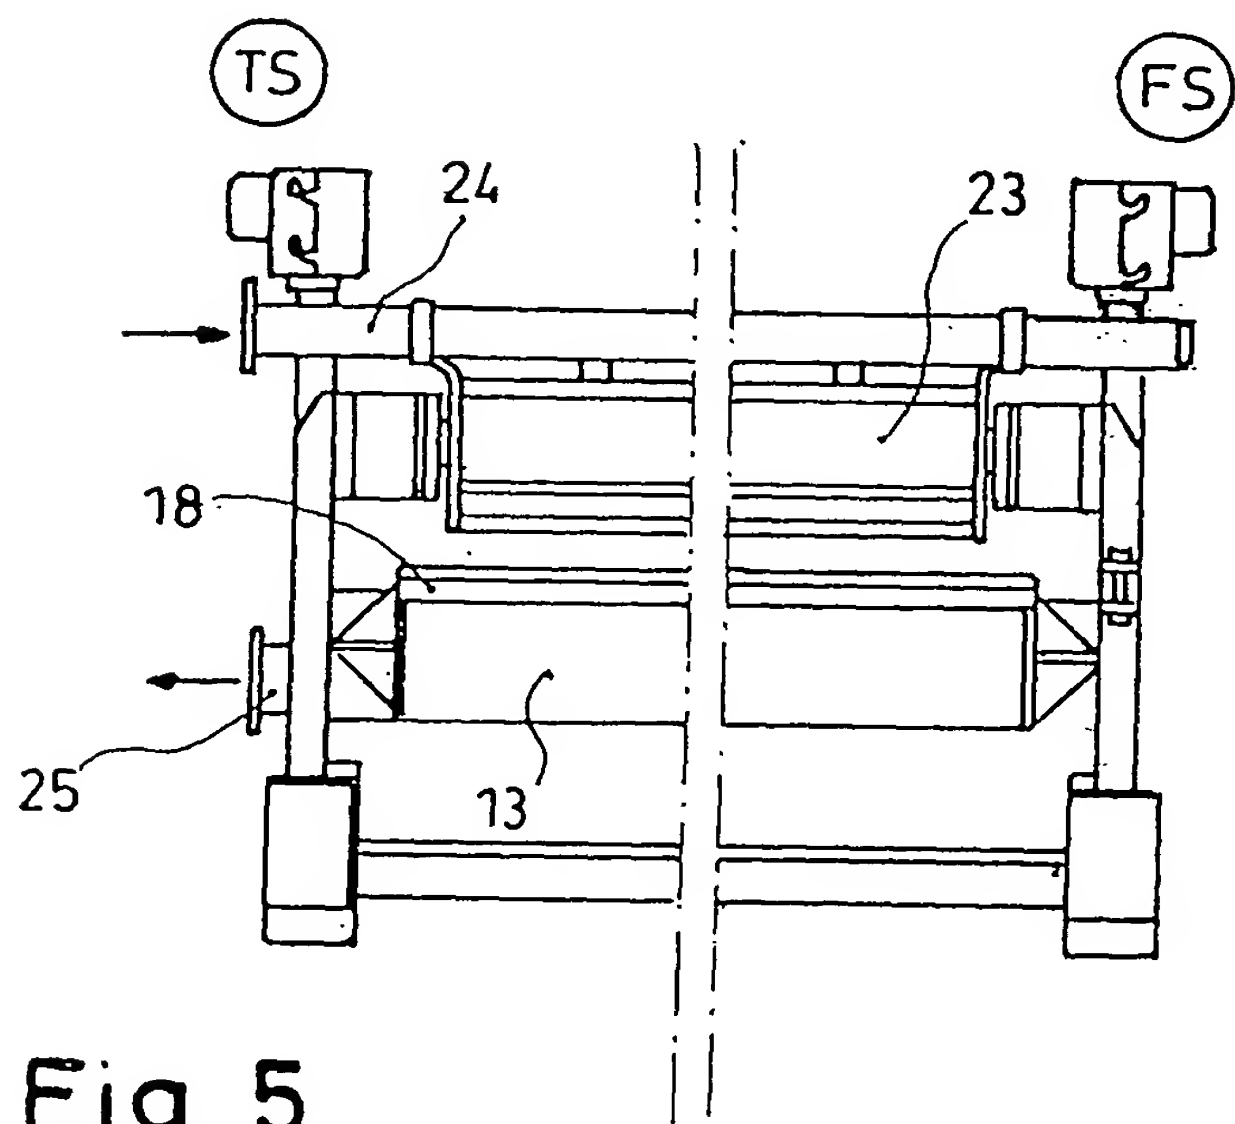


Fig. 5

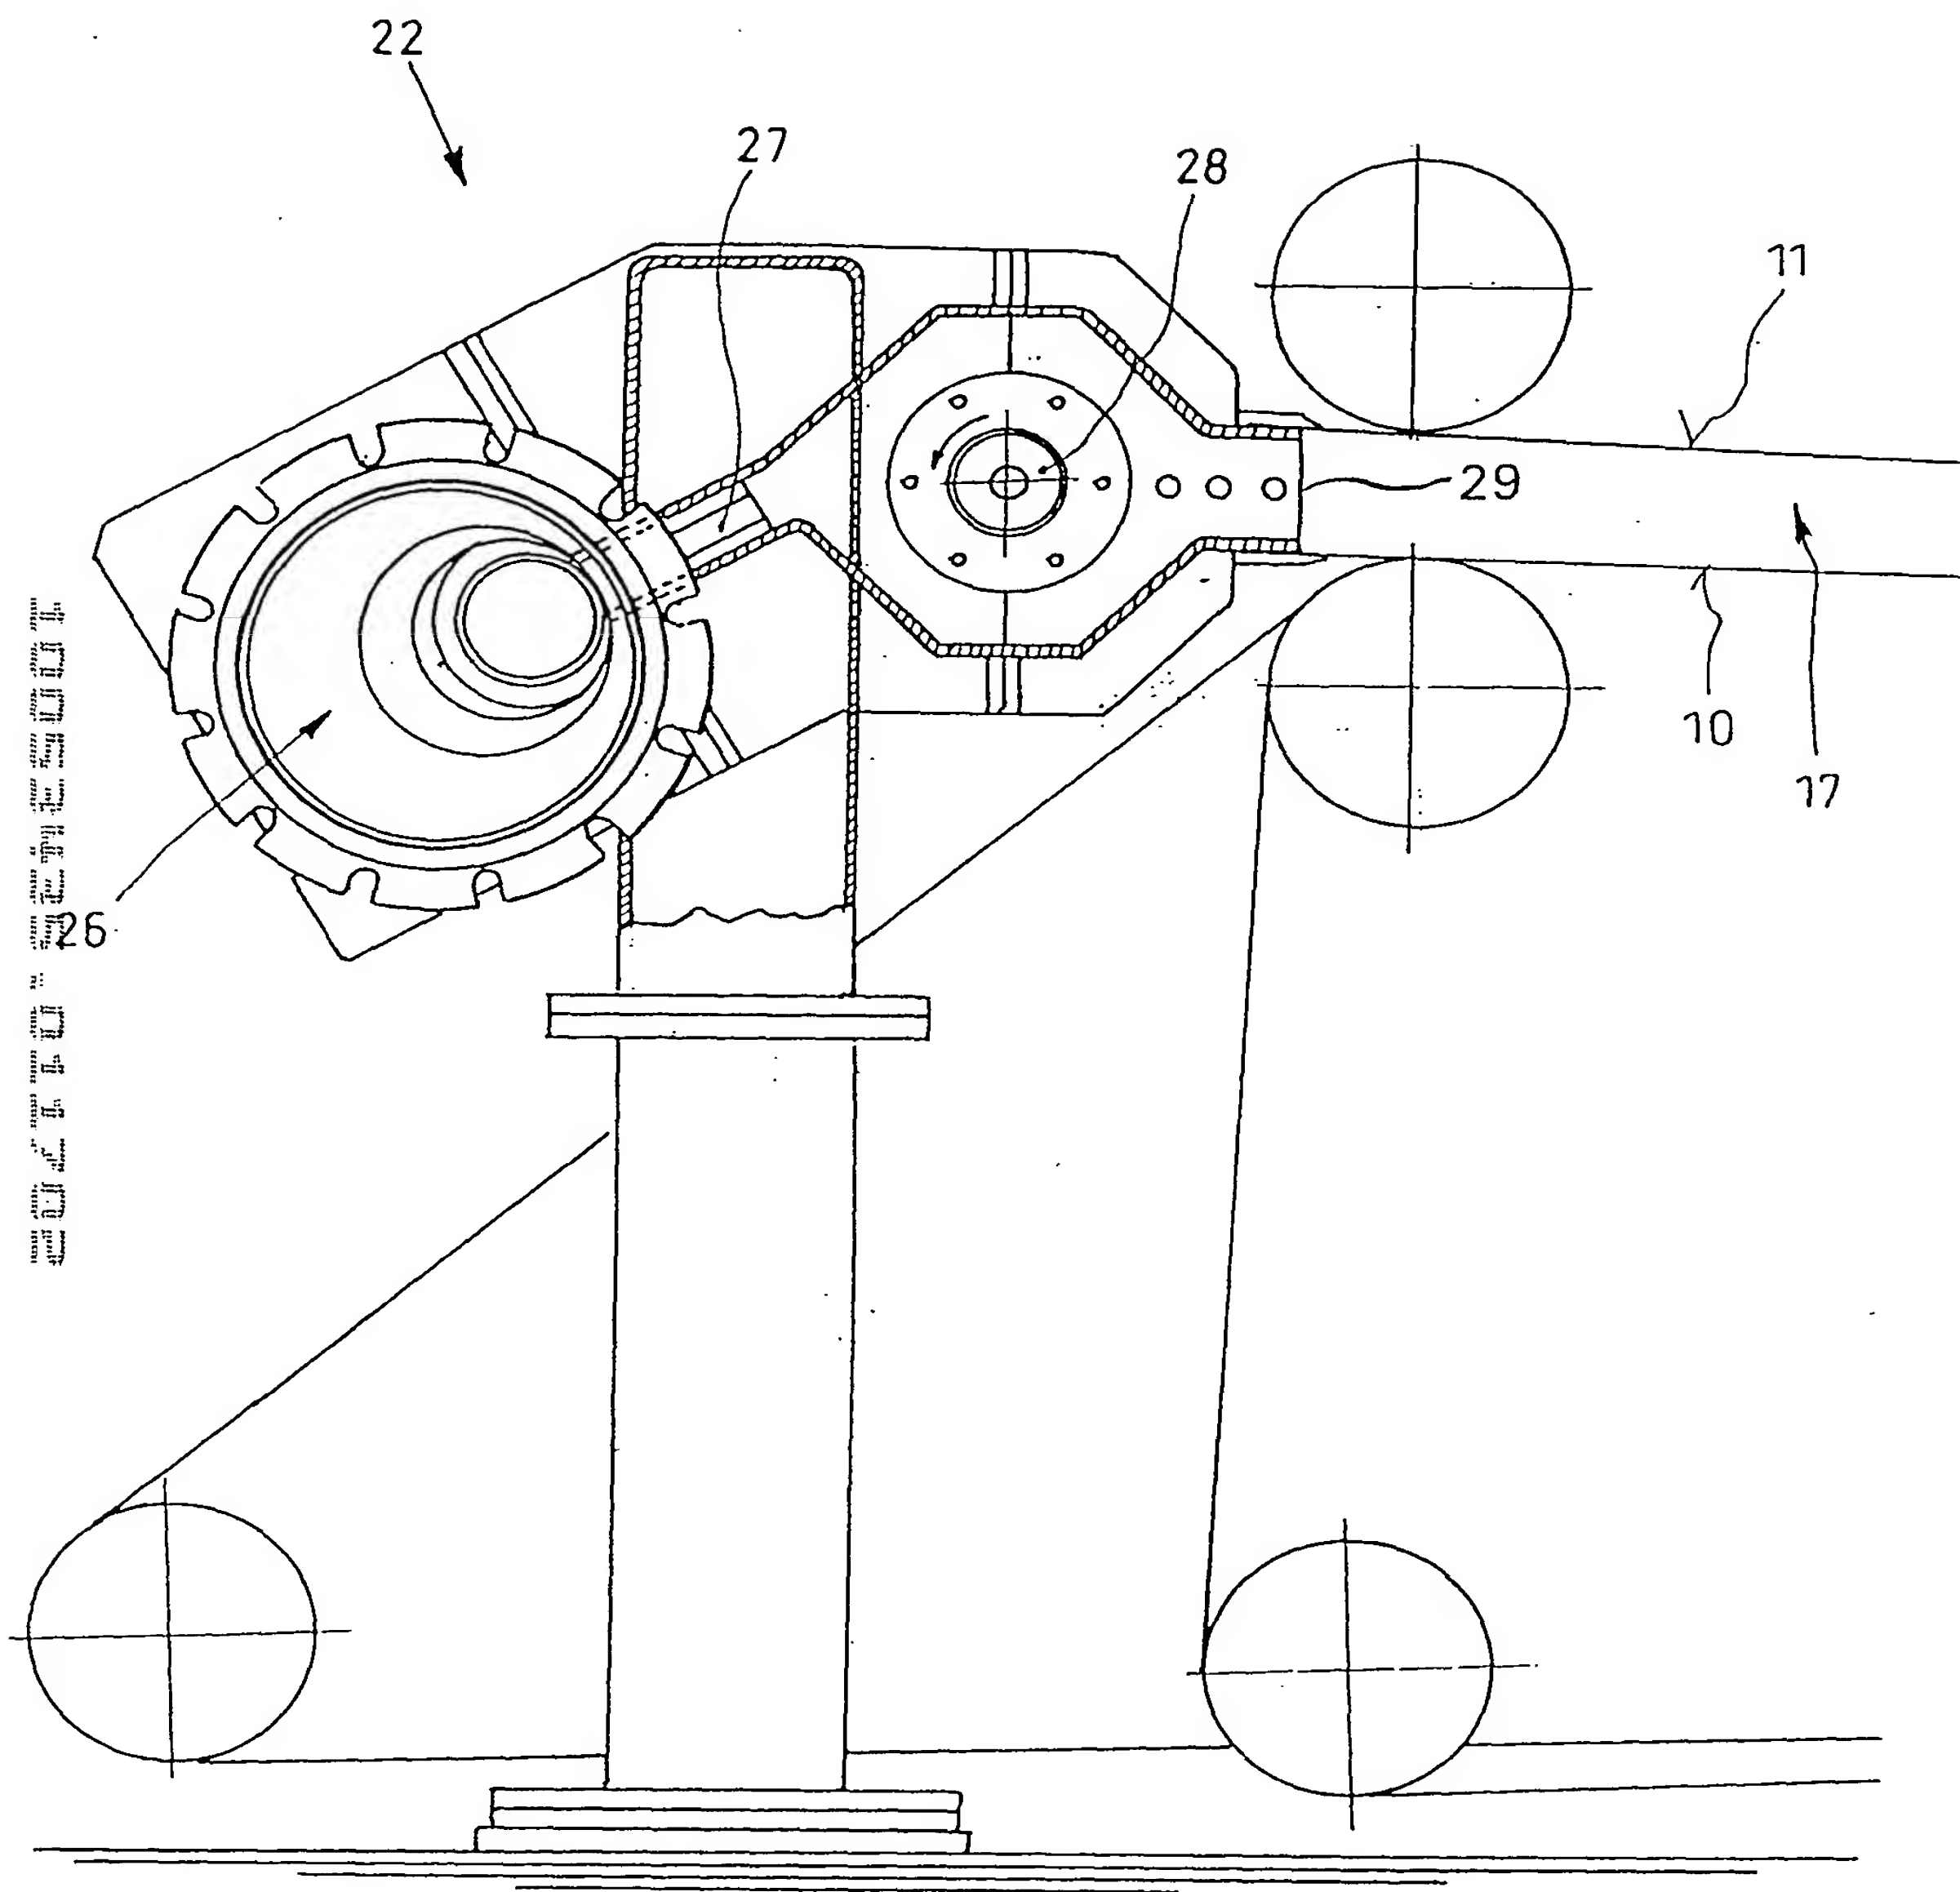


Fig. 6